



City Research Online

City St George's, University of London

Citation: Hickey, M., Samuels, N., Randive, N., Langford, R. M. & Kyriacou, P. A. (2009). Photoplethysmographic signals from human splanchnic organs using a new fibre-optic sensor. Paper presented at the Annual National Conference of the Institute of Physics and Engineering in Medicine (IPEM), 14-16 Sep 2009, Liverpool, UK.

This is the draft version of the paper.

This version of the publication may differ from the final published version. To cite this item please consult the publisher's version.

Permanent repository link: <https://city-ref-test.eprints-hosting.org/id/eprint/14293/>

Copyright and Reuse: Copyright and Moral Rights remain with the author(s) and/or copyright holders. Copies of full items can be used for personal research or study, educational, or not-for-profit purposes without prior permission or charge, unless otherwise indicated, provided that the authors, title and full bibliographic details are credited, a hyperlink and/or URL is given for the original metadata page and the content is not changed in any way. For full details of reuse please refer to [City Research Online policy](#).

Photoplethysmographic signals from human splanchnic organs using a new fibre-optic sensor

M Hickey¹, N Samuels², N Randive², R M Langford² and P A Kyriacou¹

¹School of Engineering and Mathematical Science, City University, Northampton Square, London, UK

²Anaesthetic Department, St Bartholomew's Hospital, Barts and the London NHS Trust, London UK

Background and purpose

Splanchnic organs are particularly vulnerable to hypoperfusion, and if undetected may contribute to the development of multiple organ failure [1]. Currently, there remains a need for a simple, accurate, continuous method of monitoring splanchnic perfusion pre-operatively, operatively and post-operatively [2]. As a preliminary to developing such a sensor, a new handheld photoplethysmographic (PPG) fibre-optic sensor and processing system were developed [2]. Such a sensor would allow the intraoperative assessment of splanchnic perfusion, as well as providing an evaluation of the fibre optics as a means for acquiring photoplethysmographic signals.

Method

Ethics Committee approval was obtained to study patients undergoing elective laparotomy. At an appropriate time during the procedure, the splanchnic PPG sensor was inserted into a sterile medical ultrasound cover. The sensor was then placed on the surface of each accessible organ by the surgeon (Figure 1). An identical fibre-optic sensor was also placed on the periphery (finger or toe) of each patient to facilitate comparison of the acquired PPG signals from both sites. All signals were monitored and acquired for approximately two minutes on each site. Blood oxygen saturation from a commercial finger pulse oximeter (GE Healthcare) was also simultaneously monitored and recorded.



Fig. 1. Fibre-optic splanchnic PPG probe being held on the small bowel by the surgeon during open laparotomy

Results

PPG signals of good quality were obtained from all accessible splanchnic sites (bowel, liver, stomach) from six patients during open laparotomy. Figure 2

shows typical ac red and infrared signals from the small bowel.

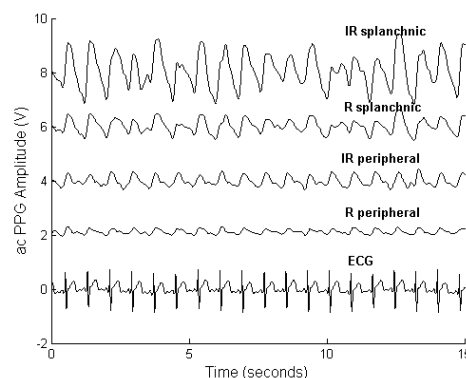


Fig. 2. Simultaneous ac infrared (IR) and red (R) splanchnic PPG signals from the small bowel and periphery

Figure 3 depicts preliminary SpO₂ results from the custom made splanchnic and peripheral fibre optic sensors and the commercial pulse oximeter. Overall there is good agreement between all pulse oximeters.

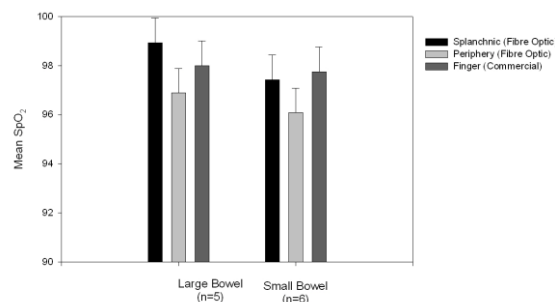


Fig. 3. Mean SpO₂ values for the large bowel and small bowel compared with simultaneous peripheral SpO₂ values acquired by the fibre optic sensor and the commercial pulse oximeter.

Conclusions

Good quality photoplethysmographic signals were obtained from all splanchnic sites in patients undergoing laparotomy. Preliminary splanchnic SpO₂ values are in good agreement with those obtained from a commercial pulse oximeter. These preliminary results suggest that the fibre optic sensor may be capable of providing a reliable means of estimating blood oxygen saturation. Further clinical trials are being conducted prior to further miniaturisation.

Acknowledgement

EPSRC

References

- [1] Jury of the Consensus, Tissue Hypoxia: How to detect, how to correct, how to prevent?, Intensive Care Med, 1996: 22, 1250-1257.
- [2] M. Hickey, and P. A. Kyriacou, Development of a New Splanchnic Perfusion Sensor, Conf. Proc. IEEE. Eng Med. Bil. Soc, 2007, 2952-5.